

Ceramic

IDENTALLOY<sup>®</sup>  
CERTIFICATE



The manufacturer certifies that the dental casting alloy provided to the laboratory with this certificate is a Predominantly Base alloy (contains less than 25%(total) Gold, Palladium and Platinum).

The laboratory certifies that Predominantly Base alloy was used to fabricate this prosthesis.

Alloy	Manufacturer	Composition
Argeloy N.P.	The Argen Corporation	Ni 76.0% Al 2.0% Cr 14.0% Be 1.8% Mo 6.0% Other <1.0%


DENTIST CERTIFICATE (attach to patient record)  
www.identalloy.org

NP – Base

Silver Palladium

Full Cast

IDENTALLOY<sup>®</sup>  
CERTIFICATE

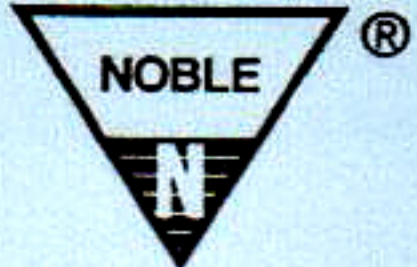

NOBLE ALLOY CONTAINS AT LEAST 25% GOLD, PALLADIUM AND PLATINUM.


The manufacturer certifies that the dental casting alloy provided to the laboratory with this certificate is a Noble alloy.

The laboratory certifies that Noble alloy was used to fabricate this prosthesis.

Alloy	Manufacturer	Composition
Select™ White	Leach & Dillon	Ag 58.46% In 2.0% Pd 24.975% Ru .025% Cu 14.5% Li .04%

DENTIST CERTIFICATE (attach to patient record)

IDENT ALLOY  
CERTIFICATE

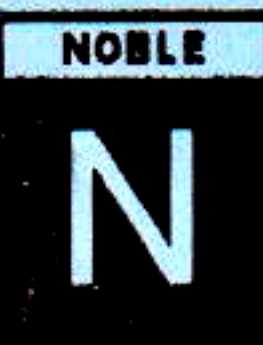

The manufacturer certifies that the dental casting alloy provided to the laboratory with this certificate is a Noble Alloy. The laboratory certifies that Noble alloy was used to fabricate this prosthesis.


ALLOY	MANUFACTURER	COMPOSITION
150 SL	Leach & Dillon	Pd 60.4% Ag 28.08% In 7.0% Sn 2.5% Ga 1.8% Li X% Ru X%

Dentist Certificate (attach to patient record)

SP

40 %

IDENTALLOY<sup>®</sup>  
CERTIFICATE

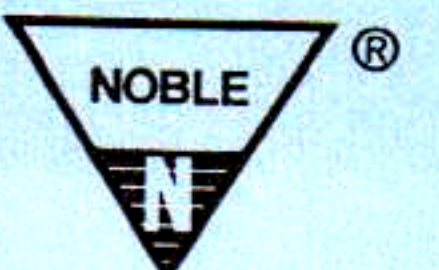

NOBLE ALLOY CONTAINS AT LEAST 25% GOLD, PALLADIUM AND PLATINUM.


The manufacturer certifies that the dental casting alloy provided to the laboratory with this certificate is a Noble alloy.

The laboratory certifies that Noble alloy was used to fabricate this prosthesis.

Alloy	Manufacturer	Composition
SELECT 40	Leach & Dillon	Au 39.9% In 1.5% Pd 4.0% Zn 1.0% Ag 45.99% Li 0.01% Cu 7.59% Ir 0.01%

DENTIST CERTIFICATE (attach to patient record)

IDENTALLOY<sup>®</sup>  
CERTIFICATE

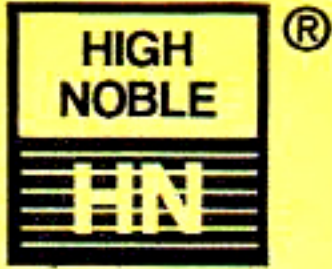

HIGH NOBLE ALLOY CONTAINS AT LEAST 40% GOLD AND 60% (TOTAL) GOLD, PALLADIUM AND PLATINUM.

The manufacturer certifies that the dental casting alloy provided to the laboratory with this certificate is a High Noble alloy.

The laboratory certifies that High Noble alloy was used to fabricate this prosthesis.


Alloy	Manufacturer	Composition
450 SL (Silhouette™ Line)	Leach & Dillon	Au 40.0% In 6.6% Pd 44.75% Li .05% Ga 1.5% Ru .2% Ag 5.0% Zn 1.9%

DENTIST CERTIFICATE (attach to patient record)

White Gold

60 %

IDENTALLOY<sup>®</sup>  
CERTIFICATE

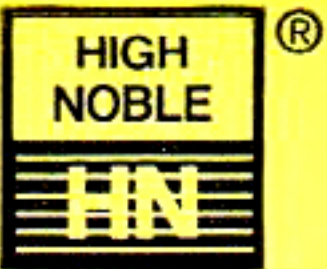

HIGH NOBLE ALLOY CONTAINS AT LEAST 40% GOLD AND 60% (TOTAL) GOLD, PALLADIUM AND PLATINUM.


The manufacturer certifies that the dental casting alloy provided to the laboratory with this certificate is a High Noble alloy.

The laboratory certifies that High Noble alloy was used to fabricate this prosthesis.

Alloy	Manufacturer	Composition
Select™60	Leach & Dillon	Au 59.9% In 1.0% Pd 3.0% Zn 0.6% Ag 26.49% Li 0.01% Cu 8.99% Ir 0.01%

DENTIST CERTIFICATE (attach to patient record)

IDENTALLOY<sup>®</sup>  
CERTIFICATE

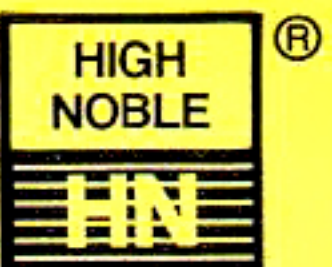

HIGH NOBLE ALLOY CONTAINS AT LEAST 40% GOLD AND 60% (TOTAL) GOLD, PALLADIUM AND PLATINUM.

The manufacturer certifies that the dental casting alloy provided to the laboratory with this certificate is a High Noble alloy.

The laboratory certifies that High Noble alloy was used to fabricate this prosthesis.

Alloy	Manufacturer	Composition
Argedent 90	The Argen Corporation	Au 89.5% Sn <1.0% Pt 5.8% Ir <1.0% Pd 1.6% In <1.0% Ag 1.2% Fe <1.0%

DENTIST CERTIFICATE (attach to patient record)  
www.identalloy.org

Yellow Gold

80 %

IDENTALLOY<sup>®</sup>  
CERTIFICATE



HIGH NOBLE ALLOY CONTAINS AT LEAST 40% GOLD AND 60% (TOTAL) GOLD, PALLADIUM AND PLATINUM.

The manufacturer certifies that the dental casting alloy provided to the laboratory with this certificate is a High Noble alloy.

The laboratory certifies that High Noble alloy was used to fabricate this prosthesis.

Alloy	Manufacturer	Composition
High Purity 77	Leach & Dillon	Au 77.0% Zn x Pt 1.0% In x Ag 13.0% Ir x Cu 8.45%

DENTIST CERTIFICATE (attach to patient record)  
www.identalloy.com